


Instruction Manual

HI 93753 Chloride ISM

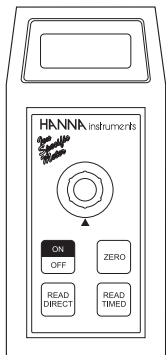

HANNA
instruments
www.hannainst.com

CE
This Instrument is in
Compliance with the CE Directives

WARRANTY

HI 93753 is warranted for two years against defects in workmanship and materials when used for its intended purpose and maintained according to instructions.

This warranty is limited to repair or replacement free of charge.

Damages due to accident, misuse, tampering or lack of prescribed maintenance are not covered.

If service is required, contact the dealer from whom you purchased the instrument. If under warranty, report the model number, date of purchase, serial number and the nature of the failure. If the repair is not covered by the warranty, you will be notified of the charges incurred. If the instrument is to be returned to Hanna Instruments, first obtain a Returned Goods Authorization Number from the Customer Service department and then send it with shipment costs prepaid. When shipping any instrument, make sure it is properly packaged for complete protection.

To validate your warranty, fill out and return the enclosed warranty card within 14 days from the date of purchase.

All rights are reserved. Reproduction in whole or in part is prohibited without the written consent of the copyright owner, Hanna Instruments Inc., Woonsocket, Rhode Island, 02895, USA.

Hanna Instruments reserves the right to modify the design, construction and appearance of its products without advance notice.

Dear Customer,

Thank you for choosing a Hanna product. This manual will provide you with the necessary information for the correct operation of the meter. Please read it carefully before using the meter. If you need additional technical information, do not hesitate to e-mail us at tech@hannainst.com.

This instrument is in compliance with CE directives EN 50081-1 and EN 50082-1.

PRELIMINARY EXAMINATION

Remove the instrument from the packing material and examine it carefully to make sure that no damage has occurred during shipment. If there is any damage, notify your Dealer.

Each Ion Specific Meter is supplied complete with

- 9V battery
- Two sample cuvettes and caps
- One transport cap

Note: Keep all packing material until the instrument has been observed to function correctly. Any defective item must be returned in its original packing.

GENERAL DESCRIPTION

The HI 93753 meter measures the chloride (Cl⁻) content in water and wastewater in the 0 to 20 mg/L (ppm) range.


The meter uses an exclusive positive-locking system to ensure that the cuvet is in the same position every time it is placed into the measurement cell.

The reagents are in liquid form and are supplied in bottles. The amount of reagent is precisely dosed to ensure maximum repeatability.

Display codes aid the user in routine operations.

The meter has an auto-shut off feature that will turn the instrument off after 10 minutes of non-use.

SPECIFICATIONS

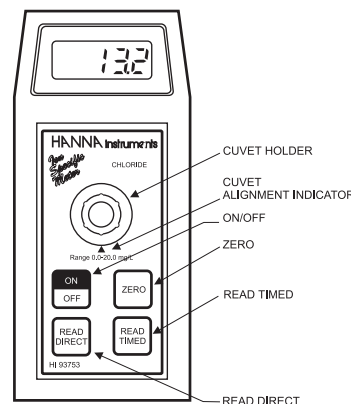

SPECIFICATIONS

Range	0.0 to 20.0 mg/L
Resolution	0.1 mg/L
Accuracy	±0.5 mg/L ±6% of reading
Typical EMC Deviation	±0.1 mg/L
Light Source	Light Emitting Diode @ 470 nm
Method	Adaptation of the mercury(II) thiocyanate method. The chloride ion displaces thiocyanate ion from mercury(II). The iron(III) present forms with thiocyanate an orange colored complex. The intensity of color is proportional to the chloride ion concentration.
Light Detector	Silicon Photocell
Environment	0 to 50°C (32 to 122°F); max 95% RH non-condensing
Battery Type/Life	1 x 9 volt/40 hours
Auto-Shut off	After 10' of non-use
Dimensions	180 x 83 x 46 mm (7.1 x 3.3 x 1.8")
Weight	290 g (10 oz.).

REQUIRED REAGENTS

Code	Description	Quantity
HI 93753A-0	Displacing Reagent	1.0 mL
HI 93753B-0	Complexing Reagent	1.0 mL

REAGENT SETS

HI 93753-01 Reagents for 100 tests and two 1 mL syringes

HI 93753-03 Reagents for 300 tests and six 1 mL syringes

DISPLAY CODE GUIDE

---	This indicates that the meter is in a ready state and zeroing can be performed.
5 IP	Sampling in Progress. This prompt appears each time the meter is performing a measurement.
-00-	This indicates that the meter is in a zeroed state and measurement can be performed.
2EAD	A zero reading was not taken. Insert a sample before adding reagent and press ZERO.
0.00	Under range. A blinking "0.00" indicates that the sample absorbs less light than the zero reference. Check the procedure and make sure you use the same cuvet for reference (zero) and measurement.
330	Over range. A flashing value higher than the maximum range (see specifications) indicates that the sample absorbs too much light and that the concentration is too high. Dilute the sample.
CAP	Light over range. The cuvet is not inserted correctly and an excess ambient light is reaching the detector. If the cover is properly installed, then contact your dealer or the nearest Hanna Customer Service Center.
L0	Light under range. The zero sample is too dark for proper zeroing. If this is not the case, contact your dealer or the nearest Hanna Customer Service Center.
V 120	The "V" indicates that the battery voltage is getting low and the battery needs to be replaced.
-BA-	This indicates that the battery is dead and must be replaced.

Note: once this indication is displayed, the meter will lockup. Change the battery to restart.

OPERATIONAL GUIDE

MEASUREMENT PROCEDURE

- Turn the meter on by pressing ON/OFF.



- When the LCD displays "---", it is ready.



- Fill one cuvette (#1) with 10 mL of distilled water (up to the mark).




- Fill another cuvette (#2) with 10 mL of sample (up to the mark).



Note: for low chloride ions concentration, rinse the cuvette a couple of times with sample before filling it with 10 mL of sample (up to the mark).

Note: for most accurate results, use two graduated pipettes to deliver exactly 10 mL of distilled water and 10 mL of sample to the cuvetts.

- Using the 1 mL syringe, add 0.5 mL of HI 93753A-0 Displacing Reagent to each cuvet.

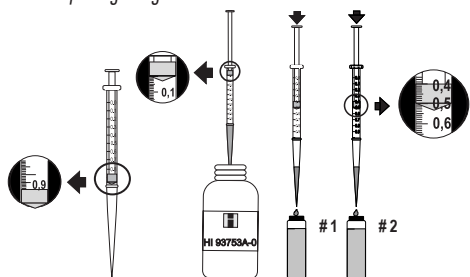


Note: to dose exactly 0.5 mL of reagent with the syringe, push the plunger completely into the syringe and insert the tip into the HI 93753A-0 Displacing Reagent bottle. Pull the plunger out until the lower edge of the seal is on the 0.0 mL mark of the syringe. Then hold the syringe above the cuvet and push the plunger down to the 0.5 mL mark.


- Replace the caps and mix each cuvet by turning the cuvette upside down for approximately 30 seconds.




- Remove the caps and use the second 1 mL syringe to add 0.5 mL of HI 93753B-0 Complexing Reagent to each cuvet.

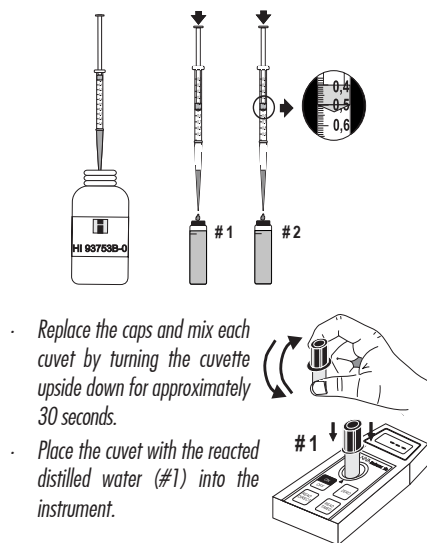


- Replace the caps and mix each cuvet by turning the cuvette upside down for approximately 30 seconds.
- Place the cuvet with the reacted distilled water (#1) into the instrument.
- Press READ TIMED and the display will show the countdown prior to zeroing the blank or, alternatively, wait for 2 minutes and press ZERO. In both cases "SIP" will appear during measurement.



- Wait for a few seconds and the display will show "-0.0-". Now the meter is zeroed and ready for measurement.



- Remove the cuvette.
- Place the other cuvet with the reacted sample (#2) into the instrument.
- Press READ DIRECT and "SIP" will blink on the LCD during measurement.



- The instrument directly displays concentration in mg/L of chloride on the Liquid Crystal Display.
- To convert the reading to mg/L of Sodium Chloride (NaCl), multiply the reading by a factor of 1.65.

INTERFERENCES

The pH of sample after addition of reagents should be about 2. For alkaline samples, neutralize before adding reagents. Intensely colored samples will cause interference, therefore they should be adequately treated before performing the test. Suspended matter in large amounts should be removed by prior filtration.

ACCESSORIES

- 2 syringes (1 mL), included in the HI 93753 reagents set.

TIPS FOR AN ACCURATE MEASUREMENT


The instructions below should be carefully followed during testing to ensure best accuracy.

- Do not touch the cuvette walls with your fingers.
- In order to maintain the same conditions during the zeroing and the measuring phases, it is necessary to close the cuvette to prevent any contamination.
- Do not let the test sample stand too long after adding the reagents or accuracy will be compromised.
- Whenever the cuvette is placed into the measurement cell, it must be completely free of fingerprints, oil or dirt. Wipe it thoroughly with HI 731318 or a lint-free cloth prior to insertion.
- It is important that the sample does not contain any debris. This would corrupt the readings.
- It is possible to take multiple readings in a row, but it is recommended that a zero reading be taken for each sample and that the same cuvette is used for zeroing and measurement.
- It is important to discard the sample immediately after the reading is taken because the glass might become permanently stained.
- Shaking the cuvette can generate bubbles in the sample, causing higher readings. To obtain accurate measurements, remove such bubbles by swirling or by gently tapping the vial.
- All the reaction times reported in this manual are referred to 20°C (68°F). As a general rule of thumb, they should be doubled at 10°C (50°F) and halved at 30°C (86°F).

BATTERY REPLACEMENT

Battery replacement must only take place in a non-hazardous area using a 9V alkaline battery.

Simply slide off the battery cover on the back of the meter. Detach the battery from the terminals and attach a fresh 9V battery while paying attention to the correct polarity. Replace the battery and the cover.



ACCESSORIES

REAGENT SETS

HI 93753-01 Reagents for 100 tests

HI 93753-03 Reagents for 300 tests

OTHER ACCESSORIES

HI 710009 Blue rubber boot

HI 710010 Orange rubber boot

HI 721310 9V battery (10 pcs)

HI 731318 Tissue for wiping cuvetts (4 pcs)

HI 731321 Glass cuvettes (4 pcs)

HI 731325 Caps for cuvettes (4 pcs)

HI 93703-50 Cuvettes cleaning solution (230 mL).

CE DECLARATION OF CONFORMITY

Recommendations for Users

Before using these products, make sure that they are entirely suitable for the environment in which they are used.

Operation of these instruments in residential area could cause unacceptable interferences to radio and TV equipments, requiring the operator to take all necessary steps to correct interferences.

Any variation introduced by the user to the supplied equipment may degrade the instruments' EMC performance.

To avoid damages or burns, do not perform any measurement in microwave ovens.

